

**PROCUREMENT OF EQUIPMENT FOR CLINIC FOR INFECTIOUS AND
TROPICAL DISEASES OF THE CLINICAL CENTER OF SERBIA
(PROCUREMENT NO. IOP/65-2022/UHI)**

CLARIFICATION NO. 3

Issued on June 22, 2022

Regarding the list of questions that the Purchaser, Public Investment Management Office Belgrade, No. 11 Nemanjina street, have received from the potential bidders, concerning the procurement procedure: Procurement of equipment for Clinic for infectious and tropical diseases of the clinical center of Serbia, no. IOP/65-2022/UHI, we give you the following answers:

Question for LOT 1:


With regard to item n. 19 "Oxygen flowmeter" please clarify:

- the type of terminal unit into which the flowmeter is to attach;
- the clearance required for the medical rail

Answer:

Terminal unit id DIN Dreager, and the medical rail is just beside, as you can see on photo



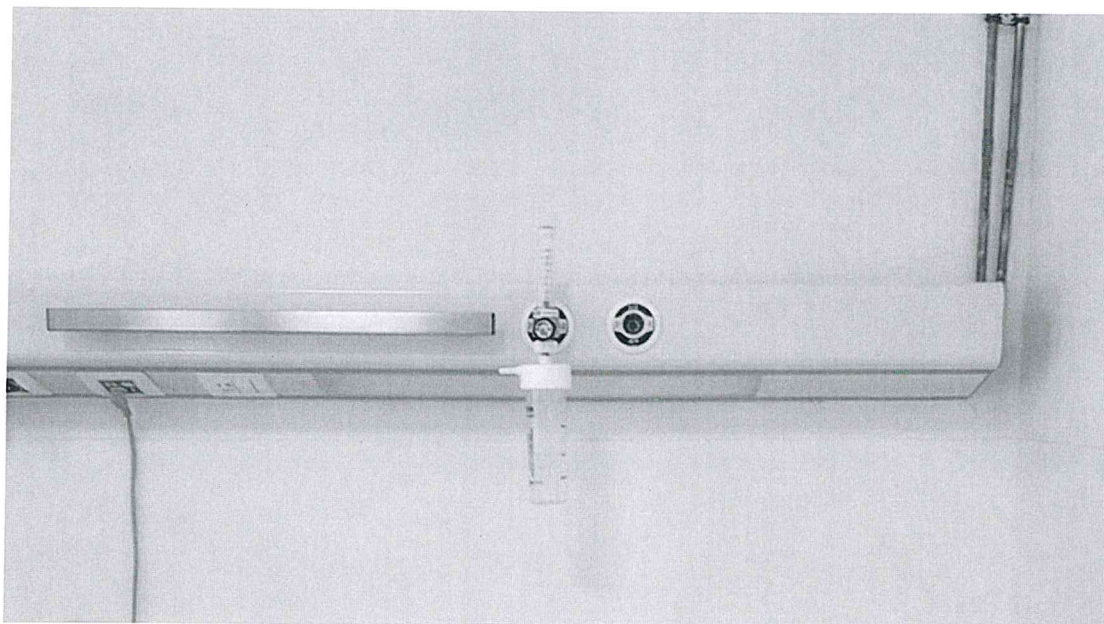

With regard to item n. 20 "Electrical Suction" please clarify
- the electrical specification of the destination country (voltage, Hz)
- the electrical plug /socket type in use.

We look forward to receiving your reply as soon as possible and we thank you for your cooperation

Answer:

Country	Plug type	National Plug Standard	Residential Voltage	Three-Phase Voltage (L-L)	Frequency
Serbia	C	JUS N.E3.552	230 V	400 V	50 Hz
	F	JUS N.E3.553			

Public Procurement Committee